

Urgent Field Safety Notice

AIMC 25-06.A.OUS

Atellica CI Analyzer
Atellica IM Analyzer
ADVIA Centaur XP System
ADVIA Centaur XPT System
ADVIA Centaur CP System

Title	Atellica IM and ADVIA Centaur Homocysteine Calibrator Instability
Date Issued	Apr-2025

Products	Product	Siemens Material Number/Unique Device Identification	Kit Lot Number	Manufacturing Date	Expiration Date
	Atellica IM Homocysteine Calibrator (2 Pack)	10995498 / 00630414598253	86236A74	14-May-2024	14-May-2025
			44206A75	25-Sep-2024	25-Sep-2025
	ADVIA Centaur HCY Calibrator (2 Pack)	10310376 / 00630414468198	86237A74	14-May-2024	14-May-2025
			44207A75	25-Sep-2024	25-Sep-2025

Issue Description Siemens Healthineers has confirmed through the investigation of customer complaints that the Atellica IM Homocysteine Calibrator and ADVIA Centaur HCY Calibrator Lots listed in the table above do not meet the assay Instructions for Use (IFU) reference interval due to calibrator instability. As the calibrator ages, homocysteine results were observed to increase with bias up to 19.2% at 8 months post manufacture.

The described calibrator instability impacts homocysteine on the Atellica CI Analyzer, Atellica IM Analyzer, ADVIA Centaur XP System, ADVIA Centaur XPT System, and ADVIA Centaur CP System.

Impact to Results Erroneously elevated homocysteine may occur as a result of this issue. A positive drift may impact both QC and patient results in all sample matrices. Figure 1 of the Appendix provides representative data that may be observed.

Based on customer complaints and investigation results, users may observe elevated homocysteine results as compared to historical patient results and/or the published or laboratory-defined reference interval.

Results of this assay should always be interpreted in conjunction with the patient's medical history, clinical presentation, and other findings.

Customer Actions

- Perform the instructions provided below:

- Please review this letter with your Medical Director to determine the appropriate course of action, including for any previously generated results, if applicable.
- Discontinue use of and discard the kit lots listed in the table above (Products Section).
- Review your inventory of these products to determine your laboratory’s replacement needs and to provide information to Siemens Healthineers for reporting to the authorities.
- Complete and return the Field Correction Effectiveness Check Form attached to this letter within 10 days.
- Please retain this letter with your laboratory records and forward this letter to those who may have received this product.


Resolution Atellica IM and ADVIA Centaur Homocysteine Calibrator Lots ending in 74 and 75 are not available for purchase. Alternate Atellica IM and ADVIA Centaur Homocysteine Calibrator lots are available at Siemens Distribution Center(s).

Single Registration Number (SRN) US-MF-000016560

We apologize for the inconvenience this situation may cause. If you have any questions, please contact your Siemens Healthineers Customer Care Center or your local Siemens Healthineers technical support representative.

Appendix Additional Data

Figure 1. Atellica IM Homocysteine Calibrator Lots ending in 74 and 75 as compared to Siemens Internal Standardization, using EDTA patient samples and commercial Quality Control (QC) Material – Percent (%) Bias Plot

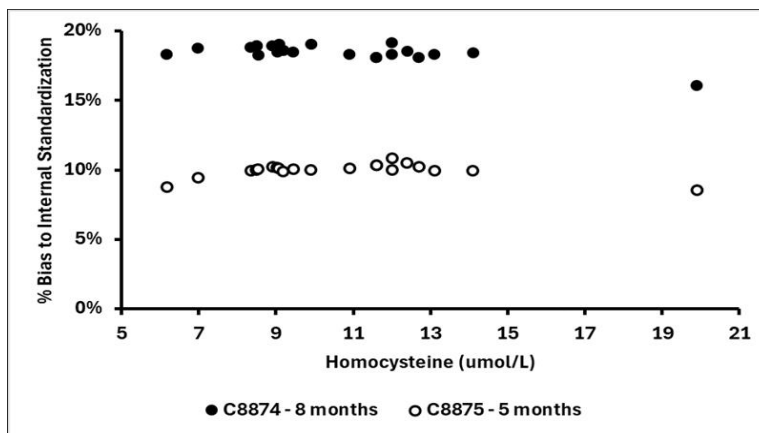

Atellica IM Homocysteine Calibrator Lots ending in 74 and 75 contain Homocysteine Calibrator Level Lots C8874 and C8875, respectively.

The number of months next to the calibrator lot represents the calibrator age at the time of testing.

These data are representative of Atellica CI, ADVIA Centaur XP, ADVIA Centaur XPT, and ADVIA Centaur CP performance.

Atellica and ADVIA Centaur are a registered trademark of Siemens Healthcare Diagnostics Inc. © Siemens Healthcare Diagnostics Inc. 2025.

Siemens Healthcare Sdn. Bhd.
 Registration No: 201501001338 (1126670-U)
 Management: Siow Ai Li, Managing Director;
 Jan Henning Tiedermann, Finance Director

Block A, Level 33A,
 Menara The MET,
 No 20 Jalan Dutamas 2,
 50480 Kuala Lumpur

Tel: +603-6206 4945
 Fax: +603-6206 5146
 siemens-healthineers.com/en-my

FIELD CORRECTION EFFECTIVENESS CHECK

This response form is to confirm receipt of the enclosed Siemens Healthineers Urgent Field Safety Notice AIMC 25-06.A.OUS dated Apr 2025. Please read each question and indicate the appropriate answer.

If you have received any complaints of illness or adverse events associated with the products listed in the table on Page 1 immediately contact your local Siemens Healthineers Customer Care Center or your local Siemens Healthineers technical support representative.

Return this completed form as per the instructions provided at the bottom of this page.

- 1. Have you read and understood the instructions provided in this letter? Yes No
- 2. Do you have the affected product(s) on hand? Please check inventories before answering. Yes No
- 3. Were affected Site Personnel notified? Yes No
- 4. Was a copy of the letter retained and posted with the current product labeling? Yes No

If the answer to the question #2 above is yes, please complete the table below to indicate the quantity of affected product in your laboratory and replacement product required.

Product Description SMN #/Lot #	Quantity of Affected Product in inventory Discarded/Replacement Quantity Required		
<i>Atellica IM Homocysteine Calibrator (2PK) SMN: 10995498 Kit Lot: 86236A74</i>			
<i>Atellica IM Homocysteine Calibrator (2PK) SMN: 10995498 Kit Lot: 44206A75</i>			
<i>ADVIA Centaur HCY Calibrator (2PK) SMN: 10310376 Kit Lot: 86237A74</i>			
<i>ADVIA Centaur HCY Calibrator (2PK) SMN: 10310376 Kit Lot: 44207A75</i>			
Name of person completing questionnaire:			
Title:			
Institution:			
Street:			
City:		State:	Zip Code:
Phone:		Country:	

Please send a scanned copy of the completed form via email to fscreportingunit.my@siemens-healthineers.com.

We apologize for the inconvenience this situation may cause. If you have any questions, please contact your Siemens Healthineers Customer Care Center or your local Siemens Healthineers technical support representative.